



## Application of the OSL technique for beta dosimetry

T.N.O. Pinto<sup>a,b</sup>, S.G.P. Cecatti<sup>a,b</sup>, C.C. Gronchi<sup>a,b</sup>, L.V.E. Caldas<sup>b</sup>

<sup>a</sup>Fundacentro, Ministério do Trabalho e Emprego, São Paulo, SP, Brazil

<sup>b</sup>Instituto de Pesquisas Energéticas e Nucleares, Comissão Nacional de Energia Nuclear, São Paulo, SP, Brazil

Received DATE; received in revised form DATE; accepted DATE

### Abstract

In recent years, the optically stimulated luminescence (OSL) technique has been used in personal dosimetry, and aluminum oxide ( $\text{Al}_2\text{O}_3:\text{C}$ ) has become a very useful material for this technique. The objective of this work was to study the dosimetric characterization of  $\text{Al}_2\text{O}_3:\text{C}$  for beta radiation detection using the OSL method. The results obtained show that for monitoring of workers exposed to beta radiation, the technique and the material are useful, but the energy dependence of the OSL response of  $\text{Al}_2\text{O}_3:\text{C}$  has to be taken into consideration.

© 2006 Elsevier Ltd. All rights reserved.

**Keywords:** Optically stimulated luminescence, beta radiation,  $\text{Al}_2\text{O}_3:\text{C}$

### 1. Introduction

When workers handle radioactive materials they may expose their extremities to doses significantly greater than the whole body dose. Beta radiation may cause damage to the workers in these cases, and then extremity dosimeters become extremely important [Durham et al, 2002].

The main requirement of a personal dosimeter for the monitoring of beta radiation doses is the capability of measuring the ICRU quantity of  $H_p(0.07)$  with satisfactory accuracy, independently of the radiation incident angle and the beta radiation energy [Akselrod et al, 1999].

Beta dosimetry presents more difficulties than gamma dosimetry, since skin dose is defined at a single depth in tissue, and the dose deposition from beta particles in tissue is highly non-uniform. Dosimeters with a finite thickness yield the dose averaged over the thickness of the dosimeter [Durham et al, 2002].

In extremity dosimetry the dose should preferably be measured using a very thin dosimeter, particularly for beta dosimetry [Akselrod et al, 1996]. Extremity dosimeters have to be produced in very thin layers with sufficient sensitivity to provide accurate dose measurements between 1 mGy and 10 Gy. Various types of thin detectors have been prepared and tested using highly sensitive thermoluminescent (TL) phosphors, e. g.  $\text{MgB}_4\text{O}_7:\text{Dy}$ ;  $\text{CaSO}_4:\text{Dy}$ ;  $\text{Al}_2\text{O}_3:\text{C}$  and  $\text{LiF:Mg,Cu,P}$  [Campos and Lima, 1987], [Akselrod et al, 1996].

Aluminum oxide ( $\text{Al}_2\text{O}_3:\text{C}$ ) was initially developed as a thermoluminescent (TL) material. In recent years, the optically stimulated luminescence technique has been used in

personal dosimetry, and  $\text{Al}_2\text{O}_3:\text{C}$  has become a material of choice for this technique [Akselrod et al, 1999].

The  $\text{Al}_2\text{O}_3:\text{C}$  detectors present very good dosimetric properties, and they have become successful personal OSL dosimeters [Akselrod et al, 1990], [McKeever et al, 1995], [McKeever, 2001]. Thin layers of this material can be used to measure different energies of beta radiation, within the limits established in the US by the National Voluntary Laboratory Accreditation Program and the US Department of Energy Laboratory Accreditation Program with acceptable accuracy [Akselrod et al, 1999].

The objective of this work is the dosimetric characterization of  $\text{Al}_2\text{O}_3:\text{C}$  for beta radiation detection using the OSL method in order to monitor workers exposed to beta radiation.

### 2. Materials and Methods

The beta irradiations of the OSL detectors were performed using the beta secondary standard system of the Calibration Laboratory at IPEN, with  $^{90}\text{Sr} + ^{90}\text{Y}$ ,  $^{85}\text{Kr}$  and  $^{147}\text{Pm}$  sources, manufactured by AEA Technology, Germany, and calibrated by the primary standard laboratory, Physikalisch - Technische Bundesanstalt (PTB), Germany. The radiation source characteristics can be seen at Table 1.

The measurements were obtained using OSL dot dosimeters of  $\text{Al}_2\text{O}_3:\text{C}$  read with the Landauer microStar reader and software. This detector is a layer of  $\text{Al}_2\text{O}_3:\text{C}$  sandwiched between two layers of polyester for a total thickness of 0.3 mm and diameter of 0.7 mm [Landauer, 2006].

For the irradiations, each OSL dot dosimeter of  $\text{Al}_2\text{O}_3:\text{C}$  was positioned on a polymethylmethacrylate (PMMA) phantom (120 mm x 120 mm x 15 mm). The dots were irradiated at the phantom surface-source distance of 30 cm in the cases of  $^{90}\text{Sr} + ^{90}\text{Y}$  and  $^{85}\text{Kr}$ , and at 20 cm in the case of  $^{147}\text{Pm}$ , because the absorbed dose rates were determined at those distances by the PTB laboratory.

The measurements were always taken immediately after irradiation. The detectors were optically treated at  $26 \times 10^3$  lux for one hour prior to being re-utilized. A Delta OHM radiometer, model D09721, LUX LP 9021PHOT sensor, was utilized to determine the light level. [Gronchi et al, 2007].

Table 1 - Characteristics of the secondary standard system of beta radiation.

Source	$^{147}\text{Pm}$	$^{85}\text{Kr}$	$^{90}\text{Sr} + ^{90}\text{Y}$
Nominal activity (MBq)	3700	3700	460
Mean beta energy (MeV)	0.06	0.69	0.80
Absorbed dose rate in air ( $\mu\text{Gy}\cdot\text{s}^{-1}$ )	$2.35 \pm 0.05$	$39.7 \pm 0.5$	$16.46 \pm 0.22$
Calibration distance (cm)	20	30	30
Reference date	19/11/2004	30/11/2004	08/12/2004

### 3. Results

#### 3.1. Reproducibility

The reproducibility of the OSL response of  $\text{Al}_2\text{O}_3:\text{C}$  detectors was obtained by taking ten measurements of each OSL dosimeter, irradiated with an absorbed dose of 0.6 mGy of beta radiation ( $^{90}\text{Sr} + ^{90}\text{Y}$ ). The reproducibility obtained of the  $\text{Al}_2\text{O}_3:\text{C}$  detectors was 2.5 % ( $1\sigma$ ).

#### 3.2. Dose response curve

The OSL dots of  $\text{Al}_2\text{O}_3:\text{C}$  were irradiated with  $^{90}\text{Sr} + ^{90}\text{Y}$  in the dose range of 0.1 mGy to 10 mGy. Ten dots were utilized for each dose level. The dose response curve presents (Fig. 1) a linear response for low doses, which are more probable to occur in occupational dosimetry. The error bars correspond to  $1\sigma$ .

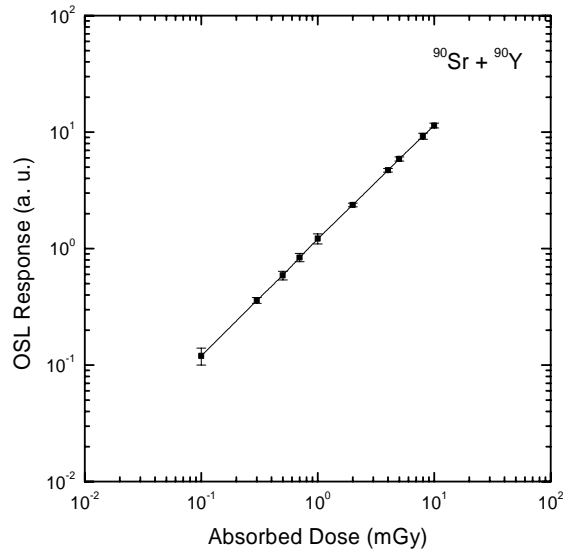


Figure 1. Dose response curve of OSL response of  $\text{Al}_2\text{O}_3:\text{C}$  dot dosimeters to beta radiation ( $^{90}\text{Sr} + ^{90}\text{Y}$ ).

#### 3.3. Energy Dependence

The OSL dot dosimeters were exposed to a dose of 3 mGy of beta radiation of  $^{90}\text{Sr} + ^{90}\text{Y}$  and  $^{85}\text{Kr}$ , and to a dose of 13 mGy of  $^{147}\text{Pm}$ . The results were normalized to the  $^{90}\text{Sr} + ^{90}\text{Y}$  mean energy and divided by the absorbed doses (Fig. 2). Due to the low radiation energy, in the case of the  $^{147}\text{Pm}$  source, the absorbed dose rate had to be corrected for the environmental standard conditions of 20°C, 101.3 kPa and 50% relative humidity. The curve was obtained using the Origin software “spline” curve correction to link the three main points. The response is given per unit dose and error bars are  $1\sigma$ . These materials present a very high dependence of the OSL response on the beta radiation energy, which has to be taken into consideration for beta monitoring. The energy dependence curve obtained for the  $\text{Al}_2\text{O}_3$  pellets irradiated with different beta sources is comparable to that presented by Akselrod et al [1999]. The energy response for beta radiation can be flattened by using filters as discussed by Akselrod et al [1996].

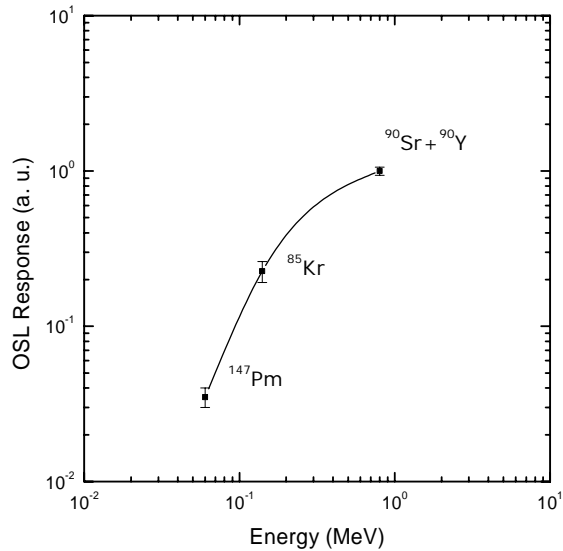


Figure 2 – Energy dependence of OSL response of Al<sub>2</sub>O<sub>3</sub>:C dot dosimeters to beta radiation.

#### 4. Conclusion

Al<sub>2</sub>O<sub>3</sub>:C dot dosimeters were characterized for beta radiation dosimetry using the OSL technique in this work. Reproducibility of OSL response was 2.5%.

The dose response curve presents a linear response in the low dose range of 0.1 mGy to 10 mGy, which are more probable to occur in occupational dosimetry.

The material presents a high energy dependence that has to be taken into consideration for beta occupational dosimetry. As discussed by Akselrod et al [1996], filters may be used to flatten this energy dependence curve.

The results on the main dosimetric characteristics investigated in this paper show that the OSL dot dosimeters may be useful for extremity dosimetry of workers exposed to beta radiation, taking the energy dependence into consideration.

#### Acknowledgements

The authors are very grateful to Fundação de Amparo à Pesquisa do Estado de São Paulo (FAPESP) and to Conselho Nacional de Desenvolvimento Científico e Tecnológico (CNPq), Brazil, for partial financial support.

#### References

- Akselrod, M. S. and Kortov, V. S., 1990. Thermoluminescent and exoemission properties of new high-sensitivity TLD  $\alpha$ -Al<sub>2</sub>O<sub>3</sub>:C crystals. *Radiat. Prot. Dosim*, 33, 123-126.
- Akselrod, M. S., McKeever, S. W. S., Moscovitch, M., Emfietzoglou, D., Durhan, J. S. and Soares, C. G. 1996, A thin-layer Al<sub>2</sub>O<sub>3</sub> beta TL detector. *Radiat. Prot. Dosim*. 66, 105-110.
- Akselrod, A., Akselrod, M. S., Larsen, N. A., Banerjee, D., Botter-Jensen, L., Christensen, P., Lucas, A. C., McKeever, S. W. S. and Yoder, R. C. 1999, Optical stimulated luminescence response of Al<sub>2</sub>O<sub>3</sub> to beta radiation. *Radiat. Prot. Dosim*. 85, 125-128.
- Campos, L. L. and Lima, M. F. 1987, Thermoluminescent CaSO<sub>4</sub>:Dy Teflon pellets for beta radiation detection. *Radiat. Prot. Dosim*. 18, 95-97.
- Durhan, J. S., Zhang, X., Payne, F. and Akselrod, M. S. 2002, Design of a finger ring extremity dosimeter based on OSL readout of alpha-Al<sub>2</sub>O<sub>3</sub>:C. *Radiat. Prot. Dosim*. 101, 65-68.
- Gronchi, C. C., Cecatti, S. G. P., Pinto, T. C. N. O. and Caldas, L. V. E., 2007. Light induced fading of the OSL response of Al<sub>2</sub>O<sub>3</sub>:C detectors. In Proceedings of the International Nuclear Atlantic Conference, September 29 to October 5, Santos, Brazil.
- Landauer, User manual InLigth Systems. Landauer, Illinois, 2006.
- McKeever, S. W. S., Akselrod, M. S. and Markey, B. G. 1996, Pulsed optically stimulated dosimetry using  $\alpha$ -Al<sub>2</sub>O<sub>3</sub>. *Radiat. Prot. Dosim*. 65, 267-272.
- McKeever, S. W. S. 2001, Optically stimulated luminescence dosimetry. *Nucl. Instr. Meth. Phys. Res. B* 184, 29-54.