

## Development of a Brazilian gamma-neutron dosimeter

SOUTO, E.B.<sup>(1,2)</sup>, CAMPOS, L.L.<sup>(1)</sup>

<sup>(1)</sup>ebsouto@prorad.com.br

<sup>1</sup> Instituto de Pesquisas Energéticas e Nucleares, IPEN-CNEN/SP

Av. Prof. Lineu Prestes, 2242 Cidade Universitária 05508-000 - Sao Paulo - SP - Brazil

<sup>2</sup> Pro-Rad Consultores em Radioproteção Porto Alegre – RG - Brazil

### Abstract

Aiming to improve the neutron dosimetry in Brazil a gamma-neutron mixed field dosimeter using the techniques of TLAD and SSNTD was developed. Commercially available materials were preferentially used. The dosimeter was projected to evaluate gamma, intermediate (Albedo) and fast neutron doses from <sup>241</sup>AmBe sources. Dosimetric properties such as gamma and neutron doses and angular responses were evaluated.

PACS: 87.53.Qc

Keywords: neutron dosimeter, SSNTD, TLAD

### Introduction

The increasing use of neutron radiation in industrial and medical applications has multiplied the number of workers potentially exposed to neutron radiation, and the personal monitoring has to be extended to mixed fields gamma-neutron.

Neutron dosimetry is a complex technique and highly neutron energy dependent. Different materials and methods has been studied and proposed to an efficient neutron dosimetry<sup>[1-2]</sup>.

The personal monitoring of Brazilian workers potentially exposed to neutron radiation is limited due to the costs of the dosimeters. Aiming to improve the neutron dosimetry in Brazil the Instituto de Pesquisas Energéticas e Nucleares, IPEN-CNEN/SP, a governmental institution, in association with PRO-RAD, a private Monitoring Service, developed a gamma-neutron mixed field dosimeter using the techniques of Albedo Thermoluminescence Dosimetry - TLAD and Solid State Nuclear Track Dosimetry - SSNTD. Low cost and commercially available materials such as polyethylene, polycarbonate and polymethylmethacrylate (PMMA) were preferentially used. The dosimeter was projected to evaluate gamma, intermediate (albedo) and fast neutron doses from  $^{241}\text{AmBe}$  sources.

### **Material and Methods**

The TL detectors chosen were the Harshaw TLD-700 (gamma sensitive) and TLD-600 (neutron sensitive) ribbons and the TL measures were performed using a Harshaw 200A/B TL reader.

The track detectors were obtained using a commercially available polycarbonate 1.5mm thick named SS-1 described in Souto, 2006<sup>[3]</sup>. The chemical etching was performed using the PEW-40 solution at 75°C during 3h<sup>[4]</sup>. A video camera connected to an optical microscope was used to track counting.

The photon irradiations with effective energy close to  $^{241}\text{Am}$  gamma energy (59.7keV) were performed using RQA 7 X-ray beam quality from industrial X-ray equipment, in free air and ambient temperature. The neutron irradiations were carried out using a  $^{241}\text{AmBe}$  source, 185 GBq, and the prototypes were displaced on an ISO slab phantom.

## Prototype Description

The dosimeter prototype (Fig. 1) consists of a sandwich of three polyethylene plates 1.0 mm thick with holes to support the detectors (TL and SSNT) and a cadmium filter between two PMMA support plates 1.5 mm thick that provides the SS-1 shielding to natural radon. The TL sensitive materials (two TLD-700/TLD-600 pairs) are positioned in the frontal and back polyethylene plates respectively, with a cadmium filter positioned between them used to shield thermal neutrons, positioned in the middle plate. The SS-1 detector is also positioned in the frontal plate. The four available TL positions can be used to diverse purposes.

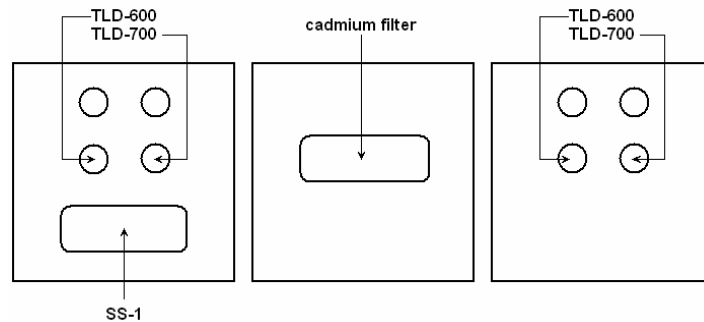


Figure 1 – Internal view of the neutron-gamma dosimeter

## Response Evaluation

Incident thermal neutrons and gamma radiation are detected by the TL detectors pair positioned in the frontal position. Albedo neutrons (intermediate neutrons backscattered by the body) are detected by the rear TL-600 detector. The cadmium filter is used to shield thermal neutrons, so incident thermal neutrons will not interact with the second TLD-600 detector nor will albedo neutrons interact with the first TLD-600 detector. Fast neutrons are detected by the SS-1 detector. The ratio between incident thermal, albedo and fast neutrons responses allows analyzing the energy spectrum to

which the dosimetry was submitted and correcting the track detector response to different radiation incidence angles.

Fig. 2 shows the dosimeter dose response to gamma radiation, incident and albedo neutrons.

The minimum detectable gamma dose, calculated according to ISO/DIS 21909<sup>[5]</sup>, is lower than 0.1 mSv.

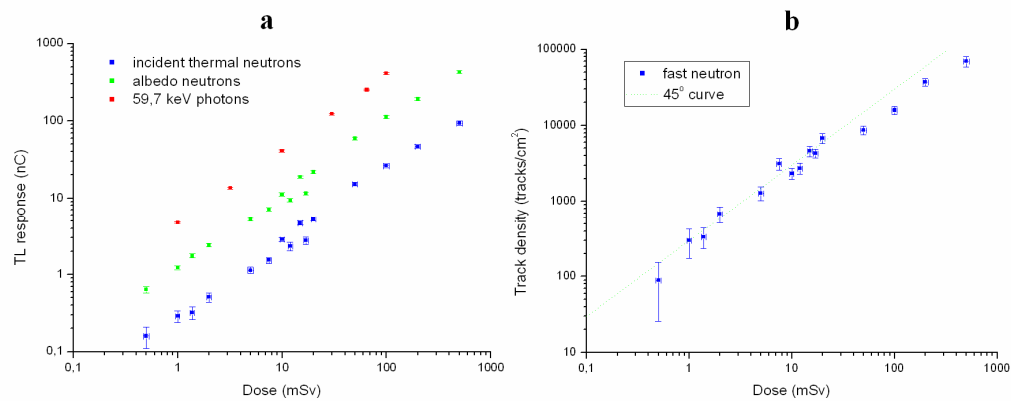


Figure 2 – a) Gamma radiation, incident and albedo neutrons dose responses;  
b) Fast neutrons dose response.

The neutron dose can be calculated utilizing only albedo or fast neutrons response. The thermal neutrons response of <sup>241</sup>AmBe sources depends on neutron moderation and scattering between source - detector.

The albedo neutron response presents linear behaviour in the studied range, whereas the fast neutron dose response is linear just between 1 and 20 mSv (Fig. 2a and 2b respectively). Above 20 mSv can be observed a saturation tendency in the SS-1 response (Fig. 2 b) . The minimum detectable fast neutron dose is 0,12 mSv and to albedo neutrons lower than 0.1 mSv.

The ratio between albedo and thermal neutron responses is constant in the studied range (0.5 to 500 mSv). This ratio provides the spectral neutron energy distribution, that is, a different ratio indicates that the dosimeter wasn't irradiated with  $^{241}\text{AmBe}$ . In the interest dose range, up to 20 mSv (ISO/DIS 21909), the variation of the ratio between fast and albedo neutrons responses is also negligible (Fig. 3).

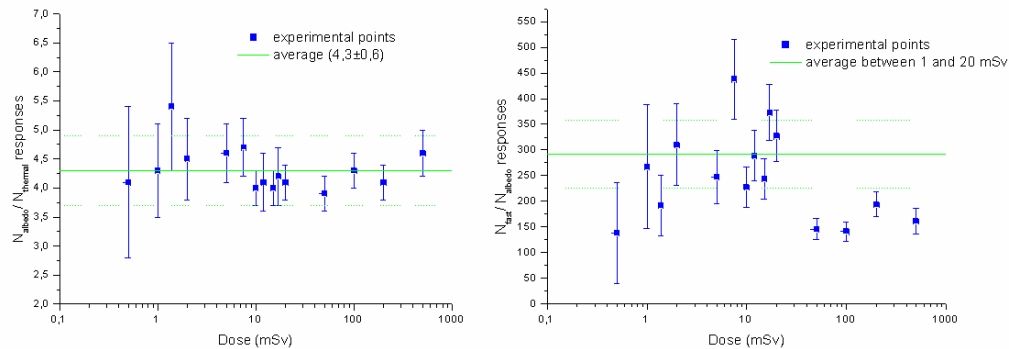


Figure 3 – Albedo to incident and albedo to fast neutron responses ratios.

The angular dependence response to thermal and albedo neutrons is acceptable (ISO/DIS 21909), instead of fast neutrons response, which can be corrected. The behaviour of fast neutron angular response seems to be a cosine function (Fig. 4). Knowing the radiation incidence angle, the SS-1 response can be corrected by a factor equal to the inverse of this angle's cosine. The incidence angle is evaluated through the variation of the ratio between fast and albedo neutron responses. This ratio presents linear behaviour as a function of the radiation incidence angle.

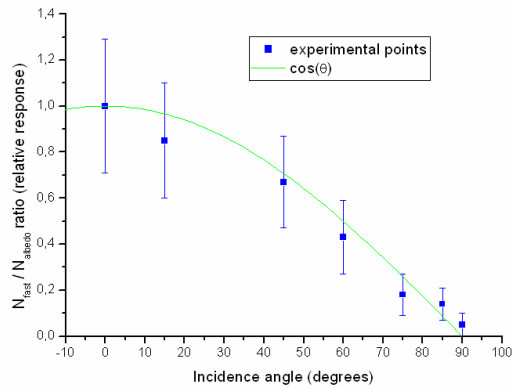


Figure 4 – Fast neutron angular dosimeter response.

The dose calculation algorithms are very simple: gamma, albedo neutrons and fast neutrons doses are estimated by linear equations extracted from the graphics of Fig. 2. Since the SS-1 track counting is very hard and tedious, the neutron dose is preferentially estimated by albedo neutrons. The fast neutron response could be used only to high doses confirmation or when TLD responses are lost .

The ratio between albedo and thermal neutron responses is constant, either under dose and angle variation. If this ratio is different from the expected value, the dosimeter was not irradiated with <sup>241</sup>AmBe or there is a scattering material between the source - dosimeter. In this case, the dose algorithms fail and can't be used.

The ratio between fast and albedo neutron responses decreases with the incidence angle, due to the high angular dependence of SS-1 response. This variation allows estimating the incidence angle and, then, correcting the fast neutron dose.

The combined use of these two dosimetric techniques, TLD and SSNTD also allows verifying the correct use of the dosimeter. A high thermal neutrons response and low fast neutron response, indicates that the dosimeter was use back turned to the source or on the user ´ back. In the same way, a high fast neutrons response and low albedo

neutrons response indicates that the dosimeter was used far from the user's body or was irradiated with no user.

## **Conclusions**

The algorithm proposed to dose estimation is very simple, but is valid only to  $^{241}\text{AmBe}$  sources; to use this dosimeter for other neutron spectrum, a new calibration is need.

The ratio between thermal, albedo and fast neutrons responses are parameters that can be used to correcting the angular dependence response and evaluating the spectrum and the correct use of the dosimeter.

The proposed dosimeter presents low cost and can easily be produced in Brazil, its performance is adequate according to ISO/DIS 21909, indicating that the dosimeter can be used to personal neutron monitoring.

## **Acknowledgements**

The authors are grateful to Pro-Rad and CNPq for the financial support and Instituto de Radioproteção e Dosimetria - IRD by making the neutron irradiations possible.

## **References**

- [1] MORELLI, B.; VILELA, E.; FANTUZZI, E. "Dosimetric performance of the fast neutron dosemeter for ENEA personal dosimetry service". *Radiat. Prot. Dosim.*, v. 85, n. 1-4, p. 105-108,1999.
- [2] FERNANDEZ, F. "Personal neutrons dosimetry in nuclear power plants using etched tracks and albedo TL dosimeters". *Radiat. Prot. Dosim.*, v. 110, n. 1-4, p. 701-704,2004.

- [3] SOUTO, E.B.; CAMPOS, L.L. “Fast neutron dose response of a commercial polycarbonate”. *Nucl. Instr. and Meth. in Phys. Res.*, to be published.
- [4] SOUTO, E.B.; CAMPOS, L.L. “Chemical etching studies of a Brazilian polycarbonate to fast neutron detection”. In. FIRST AMERICAN IRPA CONGRESS 2006, September 4-8, 2006, Acapulco. *Proceedings...*
- [5] INTERNATIONAL ORGANIZATION FOR STANDARDIZATION, *Radiation protection – Passive personal neutron dosimeter – Performance and test requirements, Standard*. Geneva: ISO, 2002. (ISO/DIS 21909).