

Uncertainty Estimation of Metals and Semimetals Determination in Wastewater by Inductively Coupled Plasma Optical Emission Spectrometry (ICP-OES)

This content has been downloaded from IOPscience. Please scroll down to see the full text.

2016 J. Phys.: Conf. Ser. 733 012023

(<http://iopscience.iop.org/1742-6596/733/1/012023>)

View [the table of contents for this issue](#), or go to the [journal homepage](#) for more

Download details:

IP Address: 200.130.19.195

This content was downloaded on 02/01/2017 at 11:36

Please note that [terms and conditions apply](#).

You may also be interested in:

[Physics of Semimetals and Narrow Gap Semiconductors – Proceedings of the Conference held in Dallas, Texas 1970](#)

A M Stoneham

[Electronic Excitation Temperature in DC Positive Streamer Discharge](#)

Wang Xiaochen, Wang Ninghui and Ding Zhenfeng

[Optical Emission Spectrometry of Plasma in Low-Damage Sub-100 nm Tungsten Gate Reactive Ion Etching Process for Compound Semiconductor Transistors](#)

Xu Li, Haiping Zhou, Chris D. W. Wilkinson et al.

[Dip and Hump Type Quantum Oscillations in Magnetoacoustic Attenuation in Semimetals](#)

Masatoshi Mori, Masao Koga and Nobuyuki Goto

[Final report on CCQM-K57: Chemical composition of clay](#)

Antonio Salas and Estele Ramírez

[Electron-Phonon Coupling and Superconductivity in Strongly Polar Semimetals](#)

Daole Yin, Rushan Han, Yuandong Dai et al.

[Corrigendum: Topological insulators, topological superconductors and Weyl fermion semimetals: discoveries, perspectives and outlooks \(2015 Phys. Scr. 2015 014001\)](#)

M Z Hasan, S-Y Xu and G Bian

[Final report on CCQM-K87: Mono-elemental calibration solutions](#)

Olaf Rienitz, Detlef Schiel, Volker Görlitz et al.

Uncertainty Estimation of Metals and Semimetals Determination in Wastewater by Inductively Coupled Plasma Optical Emission Spectrometry (ICP-OES)

J R Marques, S M Villa-Soares, T B Stellato, T B S C Silva, M G Faustino, L R Monteiro, M A F Pires, M E B Cotrim

Centro de Química e Meio Ambiente, Instituto de Pesquisas Energéticas e Nucleares (IPEN-CNEN/SP), Brazil

joyce.marques@usp.br

Abstract. The measurement uncertainty is a parameter that represents the dispersion of the results obtained by a method of analysis. The estimation of measurement uncertainty in the determination of metals and semimetals is important to compare the results with limits defined by environmental legislation and conclude if the analytes are meeting the requirements. Therefore, the aim of this paper is present all the steps followed to estimate the uncertainty of the determination of amount of metals and semimetals in wastewater by Inductively Coupled Plasma Optical Emission Spectrometry (ICP-OES). Measurement uncertainty obtained was between 4.6 and 12.2% in the concentration range of mg.L⁻¹.

1. Introduction

According to the International Vocabulary of Metrology (VIM) measurement uncertainty is a non-negative parameter characterizing the dispersion of the quantity values that is attributed to a measurand [1]. To carry out this estimation, it is necessary to follow some steps such as: to determine the measurement model; evaluate the sources of uncertainty; estimate the uncertainty in each step of the method and determine the combined and expanded uncertainty, regarding the confidence interval wanted [2].

The estimation of measurement uncertainty is important to express how precise is the method used and whether the results obtained are really meeting the needs of environmental legislations or other limits.

2. Objective

This work aims to demonstrate the steps used to estimate the measurement uncertainty in the determination of metals and semimetals (B, Sn, Cd, Ba, Cr, Cu, Fe, Mn, Ni, Pb and Ni) in wastewater, after acid digestion and analysis by ICP-OES.

3. Measurement Uncertainty

It is necessary to perform the entire method study, in order to estimate the measurement uncertainty. In this case, the method validation was performed, and all the calculations needed are described below.



3.1. Measurement Model

The first step was to determine the measurement model used to obtain the measurand. From the equation 1, it was found feasible to raise the sources of uncertainty that influences in the quantification of metals and semimetals in wastewater, using the method studied [3, 4].

$$C = \frac{(CA \times V_{final})}{V_{inicial}} \cdot \frac{1}{R} \quad (1)$$

Where: C = Concentration in the sample (mg.L^{-1}); CA = Concentration of the element according to the calibration curve (mg.L^{-1}); V_{final} = Final volume of the sample (50 mL); $V_{inicial}$ = Initial volume of the sample (45 mL); R = Recovery of the method.

3.2. Sources of Uncertainty

The uncertainty sources are presented with a quality tool called Ishikawa Diagram in Figure 1. All stages of Sample preparation and analysis were considered [5].

The contribution of each source of uncertainty is described in the next items.

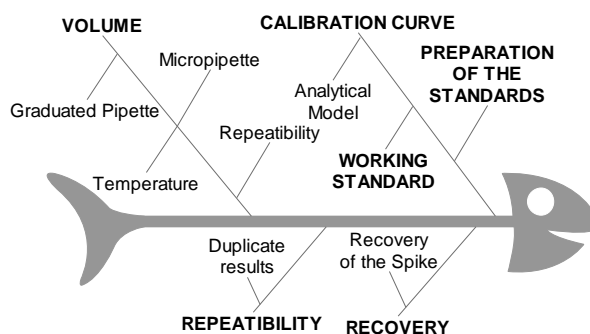


Figure 1: Ishikawa Diagram to the studied method

3.3. Volume Uncertainty

In this step, all sources of uncertainty that contribute to metal concentration dispersion were considered. Part of the uncertainty come from the volume measurement in the acid digestion process. The initial volume of sample is measured using a graduated pipette (two aliquots - 25 mL and 20 mL), after that, two acids are add to the sample, measured with a micropipette. The first source of uncertainty considered was the maximum variation of 5°C of temperature in the laboratory. This uncertainty was calculated according to equation 2 [3, 4].

$$\mu(V_T) = \frac{\Delta T \cdot Q \cdot V}{\sqrt{3}} \quad (2)$$

Where: ΔT = Variation of temperature in the laboratory ($^{\circ}\text{C}$); Q = Expansion coefficient of water ($0.000124^{\circ}\text{C}^{-1}$); V = Volume and $\sqrt{3}$ = considering rectangular distribution.

The second source of uncertainty considered was the uncertainty of the glassware, calculated according to equation 3.

$$\mu(V_P) = \frac{\mu(cert)}{\sqrt{6}} \quad (3)$$

Where: $\mu(cert)$ = Uncertainty informed by the producer and $\sqrt{6}$ = considering triangular distribution.

The last source of uncertainty of volume considered was the repeatability of the measure. In this case, ten measures were carried out, using all glassware, and the uncertainty was calculated according to equation 4 [3, 4].

$$\mu(V_{repe}) = \left(\frac{s}{\sqrt{n}} \right) \quad (4)$$

Where: s = Standard deviation of the measures and n = Number of measures.
 The volume uncertainty were combined as presented in equation 5.

$$\mu(V_X) = \sqrt{\mu(V_T)^2 + \mu(V_P)^2 + \mu(V_{repe})^2} \quad (5)$$

3.4. Calibration Curve: Preparation of Standards

All the standards used to build the calibration curves were prepared from a multielemental working standard (WS), prepared from monoelemental certified standards. To estimate the uncertainty of the preparation of WS, firstly was estimated the uncertainty of volume, as presented before, and the other sources are presented in equation 6 [3, 4].

$$\mu(C_{WS}) = \left[\sqrt{\left(\frac{\mu V_P}{V_P} \right)^2 + \left(\frac{\mu V_{VF}}{V_{VF}} \right)^2 + \left(\frac{\mu C_{std}}{C_{std}} \right)^2} \right] \cdot C_{WS} \quad (6)$$

Where μVP = Uncertainty of the volume used of the certified standard; VP = Volume used of the certified standard; μVVF = Uncertainty of the volumetric flask; VVF = Volume of the volumetric flask; $\mu Cstd$ = Uncertainty informed in the certificate of the standard; $Cstd$ = Concentration of the standard (informed in the certificate); CWS = Final concentration of the working standard.

In equation 7, it is presented the method used to estimate the uncertainty of each standard used to build the calibration curve [3, 4].

$$\mu(C_{PX}) = \left[\sqrt{\left(\frac{\mu V_P}{V_P} \right)^2 + \left(\frac{\mu V_{VF}}{V_{VF}} \right)^2 + \left(\frac{\mu C_{WS}}{C_{WS}} \right)^2} \right] \cdot C_{SX} \quad (7)$$

Where: C_{SX} = Final concentration of each standard.

Results were presented as a percentage, and the greater one was found to be the preparation of the calibration curve uncertainty.

3.5. Calibration Curve: Analytical Model

The uncertainty of the analytical model was estimated using the calculation presented in the EURACHEM Guide (equation 8) [3, 5].

$$\mu(C_X) = \frac{S}{B_1} \left[\sqrt{\frac{1}{p} + \frac{1}{n} + \frac{(C_X - \bar{C})^2}{S_{xx}}} \right] \quad (8)$$

Where: S = Residual standard deviation; B_1 = slope; p = Number of measures to determine C_X ; n = Total number of replicates; C_X = Sample concentration; \bar{C} = Calibrations average and $S_{xx} = \sum_{i=1}^n (C_i - \bar{C})^2$ where C_i = Concentration obtained from the calibration curve.

3.6. Repeatability Uncertainty

To estimate the repeatability uncertainty was used the equation 9 [3, 4].

$$\mu(Repe) = \left(\frac{Máx RSD}{\sqrt{n}} \right) \quad (9)$$

Where: $Máx DPR$ = Greater value of relative standard deviation of the interval;

In this work, data from the analysis performed in 2013 and 2014 applying this method were used.

3.7. Recovery Uncertainty

To estimate the recovery uncertainty the equation 10 was used [3, 4].

$$\mu(Rec) = \left(\frac{\overline{Rec}}{\sqrt{s}} \right) \quad (10)$$

Where: \overline{Rec} = Recovery average and s = Standard deviation of the recovery.

In this work data from the spikes analyzed in 2013 and 2014 applying this method were used to estimate the recovery of the method.

3.8. Combined and Expanded Uncertainties

The standard uncertainties were combined using the equation 11 [3, 4].

$$\mu(Conc_{Am}) = \left[\sqrt{\left(\frac{\mu V}{V} \right)^2 + \left(\frac{\mu PX}{100} \right)^2 + \left(\frac{\mu C_x}{C_x} \right)^2 + \left(\frac{\mu Repe}{100} \right)^2 + \left(\frac{\mu Rec}{100} \right)^2} \right] \cdot C_s \quad (11)$$

Where: CS = Concentration of the element in the sample.

To obtain the result of the expanded uncertainty, the results of combined uncertainty have to be multiplied by the expansion factor (k), to results with 95% of confidence interval $k = 2$.

4. Results and Discussion

Using the calculations described above the measurement uncertainty was estimated. Results of each source of uncertainty, combined uncertainty and expanded uncertainty are presented in table 1. The uncertainty source that contributes the most to all expanded uncertainties is the recovery. However, as was considered a study of 2 years to this source, the results can be considered more conservative and comprehensive.

In table 1 all the standard uncertainties ($\mu(x)/x$) are without measurement unit, due to it is adimensional it is possible combine it after all the individual steps.

Table 1: Results of standard, combined and expanded uncertainty in the studied method.

	$\mu (x)/x$						Expanded Uncertainty		
	V	Prep.	C _o	Rep	Rec	C _o (mg.L ⁻¹)	μ comb. (mg.L ⁻¹)	U (mg.L ⁻¹)	U (%)
B	0.00122	0.00792	0.01200	0.00463	0.03014	0.2499	0.0084	0.0169	6.75
Sn	0.00122	0.00847	0.01116	0.00701	0.03181	1.5230	0.0540	0.1081	7.10
Cd	0.00122	0.00803	0.00792	0.00726	0.02756	0.1260	0.0039	0.0077	6.13
Ba	0.00122	0.00893	0.00875	0.00378	0.01888	2.9710	0.0683	0.1366	4.60
Cr	0.00122	0.00851	0.01603	0.01844	0.02713	0.8110	0.0304	0.0608	7.50
Cu	0.00122	0.00807	0.00869	0.00705	0.02975	0.9210	0.0302	0.0604	6.56
Fe	0.00122	0.00841	0.00621	0.00492	0.06001	3.0610	0.1871	0.3742	12.23
Mn	0.00122	0.00794	0.01101	0.00391	0.02226	0.2725	0.0072	0.0144	5.28
Ni	0.00122	0.00892	0.00391	0.00385	0.02605	0.2555	0.0072	0.0144	5.62
Pb	0.00122	0.00807	0.01425	0.01077	0.04630	0.7720	0.0388	0.0776	10.06
Zn	0.00122	0.00839	0.00617	0.00170	0.03210	0.3243	0.0110	0.0219	6.76

5. Conclusion

Evaluating the results is possible to conclude that using data from validation process, EURACHEM guide [3, 5] and the analyst knowledge was possible to estimate, firstly, the sources of uncertainty involved in the determination of metals in wastewater, and the expanded uncertainty of each element.

The uncertainty measured is in between 4.6% and 12.2% of the concentration determined, what is coherent with the method used.

References

- [1] JCGM, International Vocabulary of Metrology - Basic and General Concepts and Associated Terms (VIM), 2012.
- [2] S. YENISOY-KARAKAS, "Estimation of uncertainties of the method to determine the concentration of Cd, Cu, Fe, Pb, Sn and Zn in tomato paste samples analysed by high resolution ICP-MS," Food Chemistry, pp. 1555 - 1561, 2011.
- [3] S L R Ellison and A Williams (Eds). Eurachem/CITAC guide: Quantifying Uncertainty in Analytical Measurement, Third edition, (2012) ISBN 978-0-948926-30-3. Available from www.eurachem.org.
- [4] H. A. FURUSAWA, "Estimativa de incerteza em análise química," 2007 São Paulo.
- [5] INMETRO, Avaliação de dados de medição: Guia para expressão de Incerteza de medição - GUM, Duque de Caxias: INMETRO/CICMA/SEPIN, 2008, p. 141.